

## Navigated Cementoplasty With O-Arm and Surgivisio: An Ambispective Comparison With Radiation Exposure

Marc Prod'homme, Jérôme Tonetti, Duccio Boscherini, Guillaume Cavalié, Gael Kerschbaumer, Didier Grasset and Mehdi Boudissa

*Int J Spine Surg* published online 16 September 2022  
<https://www.ijssurgery.com/content/early/2022/09/13/8348>

This information is current as of May 10, 2025.

---

**Email Alerts** Receive free email-alerts when new articles cite this article. Sign up at:  
<http://ijssurgery.com/alerts>

# Navigated Cementoplasty With O-Arm and Surgivisio: An Ambispective Comparison With Radiation Exposure

MARC PROD'HOMME, MD<sup>1</sup>; JÉRÔME TONETTI, MD, PhD<sup>2</sup>; DUCCIO BOSCHERINI, MD, PhD<sup>1</sup>;  
GUILLAUME CAVALIÉ, MD, MSc<sup>2</sup>; GAIL KERSCHBAUMER, MD<sup>2</sup>; DIDIER GRASSET, MD<sup>1</sup>; AND  
MEHDI BOUDISSA, MD, PhD<sup>2</sup>

<sup>1</sup>Clinic La Source, Neuro Orthopedic Center, Lausanne, Switzerland; <sup>2</sup>Orthopedic Surgery Department, University Hospital of Grenoble, La Tronche, France

## ABSTRACT

**Background:** Vertebral compression fractures (VCF) are usually treated by cementoplasty. Computerized navigation allows more accurate surgery without additional imaging acquisition for guidance and related radiation exposure. New technologies trend to optimize the irradiation for patients and surgeons. The objective was to investigate the radiological results and radiation exposure of O-arm navigation compared with the all-in-one 2-dimensional/3-dimensional (2D/3D) Surgivisio device in navigated cementoplasty procedures.

**Methods:** Patients in the O-arm group comprised an O-arm prospective cohort as well as previous patients. Operations for VCF by navigated cementoplasty took place over 18 months. Patients in the Surgivisio group were the first patients operated on using Surgivisio and were prospectively recruited. Demographic, operative, and irradiation data were collected, as well as the image quality subjectively evaluated by the surgeon. The vertebral filling was evaluated using the Garnier classification and quoted as satisfactory, acceptable, or poor. The effective dose in millisievert (mSv) was calculated for radiation exposure estimation, and the absolute risk of cancer (AR) in percent equivalent to a whole-body irradiation was also calculated.

**Results:** A total of 123 patients were included: 62 in the O-arm group and 61 in the Surgivisio group. A total of 166 vertebrae were analyzed. Compared with the Surgivisio group, the effective dose was significantly higher in the O-arm group, with a mean of 11.47 vs 1.14 mSv, respectively ( $P < 0.001$ ). The 2D part of the effective dose received by the surgeon was significantly higher in the O-arm group, with an average of 2.25 vs 0.47 mSv, respectively ( $P < 0.001$ ). Overall AR followed the same trend, with a mean of  $4.9 \times 10^{-4}\%$  in the O-arm group and  $5.7 \times 10^{-5}\%$  in the Surgivisio group ( $P < 0.001$ ). Operative time was significantly higher in the O-arm group (34.52 vs 30.12 minutes respectively,  $P = 0.03$ ). Image quality was similarly sufficient in 3D, but in 2D, image quality was significantly better in the O-arm group ( $P = 0.01$ ). Vertebral filling was significantly better in the O-arm group, with 100% of results reported as satisfactory and acceptable versus 85% in the Surgivisio group ( $P < 0.001$ ).

**Conclusions:** The O-arm delivered a 10-times higher effective dose during navigated cementoplasty in comparison with the Surgivisio device. The O-arm also had a longer operative time, but it had better image quality and radiological results.

**Level of Evidence:** 4.

New Technology

Keywords: O-arm, Surgivisio, navigation, radiation exposure, cementoplasty

## INTRODUCTION

Vertebral compression fractures (VCF) are frequent injuries, mostly related to high energy traumas on young people and bone fragility in the elderly population.<sup>1</sup> VCF are successfully treated by cementoplasty, such as vertebroplasty or kyphoplasty.<sup>2,3</sup> These procedures require the use of 2-dimensional (2D) imaging for intraoperative control of fracture reduction and cement filling. The 3-dimensional (3D) imaging with computerized navigation offers confidence and ergonomics during surgery with more accurate procedures.<sup>4</sup> However, imaging devices

currently use x-ray technology and thus have associated cancer risk,<sup>5</sup> which is referred to as “stochastic risk.” This risk can be estimated through the effective dose in millisievert (mSv). New technological advances trend to optimize irradiation related to the imaging devices.<sup>6</sup> O-arm with navigation (Medtronic, Minneapolis, MN, USA)<sup>7,8</sup> and Surgivisio (eCential Robotics, Gières, France)<sup>9,10</sup> showed good results and accuracy during spine procedures.

The purpose of this study was to compare the irradiation and radiological results of percutaneous cementoplasty for VCF performed with the O-arm surgical system associated to the navigation with

the all-in-one 2D/3D imaging device with integrated navigation named Surgivision. Hypotheses were that considering the new Surgivision device, O-arm produces more irradiation with less image quality with radiological results similar to Surgivision.

## METHODS

### Inclusion and Exclusion Criteria

The O-arm group was composed of 30 patients prospectively recruited and a review of medical records of all consecutive patients who underwent cementoplasty during a previous 18-month period at a private clinic with a fellowship program. The Surgivision group was prospectively constituted with the first consecutive patients operated at the University Hospital of Grenoble with the Surgivision device. Exclusion criteria were refusal to participate and lack of information to calculate the radiation exposure.

### Study Design

Study design was ambispective.

### Ethical Statement

The study was performed in accordance with the canonical Ethical Commission of Vaud and the approved research protocol (No. 2021–00298). All patients provided written consent for participation in the study.


### Interventions

For both groups, patients underwent operations in the prone position under general anesthesia and after

antibiotic prophylaxis. For O-arm procedures, a pin was introduced in the posterior iliac crest with patient frame attached (Figure 1). The 2D acquisitions for vertebral landmarking were performed. Then, while the detection camera could reach the patient frame and detectors on the O-arm machine (Figure 1), a 3D acquisition could be performed under medically induced apnea, and the images were transmitted to the Stealth navigation system (Medtronic, Minneapolis, MN, USA).

For the Surgivision group, the patient frame was attached using 2 to 4 Kirschner wires introduced in the spinous processes of the area of the vertebra to be operated,<sup>11</sup> and 2D fluoroscopic landmarking was performed (Figure 2). When detection of all detectors inside the patient frame was reached in an anterior-posterior view, a lateral view was performed, and then the 3D acquisition took place without apnea, the detectors following breath movements of the patient. Considering the 2 machines, operating room personnel could leave the operating room during 3D acquisition, avoiding irradiation. Then, a percutaneous cannulated navigated Jamshidi needle could be introduced inside the pedicle of the fractured vertebra (Figures 3 and 4), and cementoplasty was performed under 2D imaging. The surgeon and other personnel carried a lead apron and a thyroid shield for radiation protection.

In patients with a loss of height of the operated vertebra of more than 20% and a local kyphosis of more than 10°, vertebral augmentation was performed using a balloon Kyphon (Medtronic, Minneapolis, MN, USA)<sup>12</sup> for the O-arm group or a SpineJack device (Vexim, Balma, France)<sup>13</sup> for the Surgivision group, and then polymethyl methacrylate cement was injected

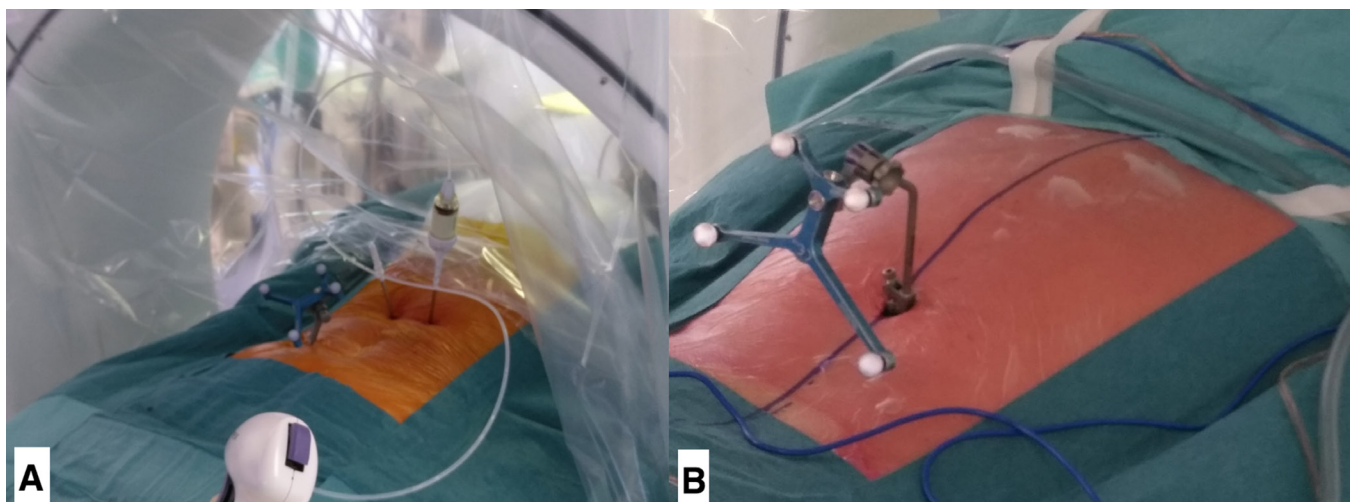

**Figure 1.** Intraoperative views of the patient frame and the O-arm settings. We can notice the percutaneous insertion of the Jamshidi needles, and the cement filler fixed on its extremity. Note the pin within the posterior cresta iliaca (A). In case of thoracic spine procedure, a spinous clamp may be required (B).




**Figure 2.** Intraoperative view of the patient frame fixed with Kirschner wires on spinous processes and a navigated Jamshidi needle with Surgivision.

in the vertebral body. In other cases for both groups, polymethyl methacrylate cement was injected alone for standard vertebroplasty. For the O-arm group, X'Pede cement was used (Medtronic, Minneapolis, MN, USA), and VertaPlex HV cement (Stryker, Portage, MI, USA) was used for the Surgivision group.

## Data Collection

Demographic data were stored such as age (in years), gender, height (in centimeters), and weight (in kilograms). Surgical data were also collected, such as the Magerl classification<sup>14</sup> of the vertebral fractures, the level and the number of operated vertebrae, the operative duration from incision to closure (in minutes), the full 2D imaging duration (in seconds), the surgeon level (junior, such as a resident or registrar or fellow, and senior), and the image quality in 2D and 3D during the procedure, reported as sufficient or insufficient according to the surgeon's consideration. We also collected irradiation data such as the dose-area product (DAP) in  $\text{mGy}\cdot\text{cm}^2$  from the dosimetric report of the Surgivision device and of the 2D O-arm fluoroscopy and the dose-length product (DLP) in  $\text{mGy}\cdot\text{cm}$  for the O-arm in 3D mode at the end of the surgical procedure. The effective dose E in mSv was calculated using the DAP and the operative field dimensions, with weight and height of the patient, through a Monte Carlo simulation using the

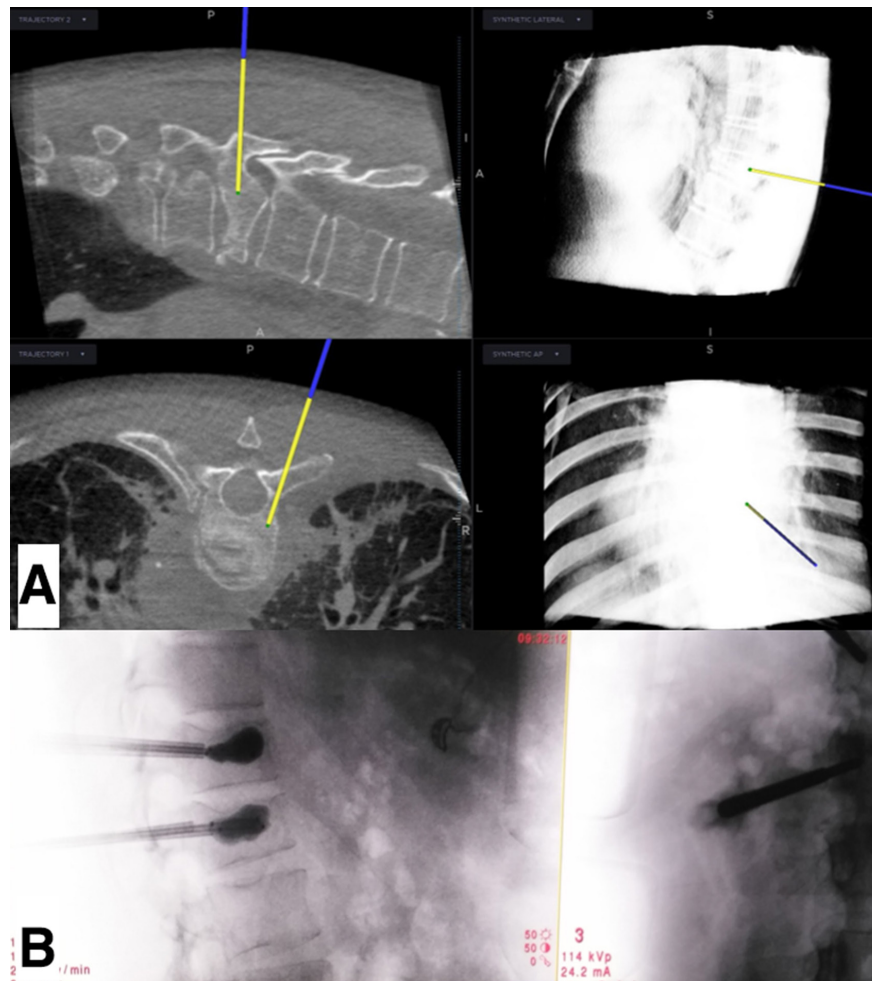

**Figure 3.** Displayed view of the computerized navigation with O-arm for percutaneous cementoplasty (A). The 2-dimensional view of balloon reduction for percutaneous kyphoplasty (B).





**Figure 4.** Displayed view of the computerized navigation with Surgivision for percutaneous cementoplasty.

**Table 1.** Patient demographics and surgery data.

Variable	O-Arm Group (n = 62)	Surgivision Group (n = 61)	P Value
Sex ratio, men/women	24/38	24/37	>0.99 <sup>a</sup>
Age, y	75 ± 11 (43–90)	69 ± 14 (36–94)	0.01 <sup>b</sup>
Body mass index, kg/m <sup>2</sup>	25.05 ± 4.37 (17.11–39.09)	24.73 ± 5.46 (15.82–48.28)	0.72 <sup>b</sup>
Operative time, min	34.52 ± 12.27 (15–90)	30.12 ± 9.36 (17–60)	0.03 <sup>b</sup>
Operative time per level, min	28.75 ± 9.71 (15–60)	24.16 ± 9.19 (8.5–54)	0.01 <sup>b</sup>
No. of cemented vertebrae	81	85	-
No. (%) of vertebroplasties	52 (64)	79 (93)	-
No. (%) of vertebral augmentations	29 (36)	6 (7)	-
No. (%) of unipedicular approaches	34 (42)	69 (81)	<0.001 <sup>a</sup>
Surgeon experience ratio, junior/senior	24/38	11/50	0.02 <sup>a</sup>

Data presented as mean ± SD (range) unless otherwise indicated.

<sup>a</sup>Fisher exact test.

<sup>b</sup>Student *t* test.

PCXMC 2.0 software (STUK, Radiation and Nuclear Safety Authority, Helsinki, Finland).<sup>15</sup> The 3D-related E was calculated with the DLP according to the European Guidelines for Multislice Computed Tomography<sup>16</sup> using the corresponding generalized coefficients *k* (in mSv/[mGy·cm]) related to the irradiated region. For the thoracic region, *k* was 0.014, for the lumbar region and the whole trunk, *k* was 0.015. The calculation formula was as follows:  $E = DLP \times k$ , where *E* is the effective dose. For approximate calculation of the effective dose related to 2D irradiation, we also utilized conversion factors *w* (in mSv/[Gy·cm<sup>2</sup>]) according to the European Commission report No. 180,<sup>17</sup> with *w* of 0.19 and 0.26 for the thoracic and lumbar spine, respectively. We also compared these results with those obtained with PCXMC. The absolute risk of cancer (AR) in percent

**Table 2.** Garnier classification of vertebral filling and cement leakage.

Radiological Classification	O-arm Group (n = 62)	Surgivision Group (n = 61)	P Value <sup>a</sup>
Cement filling			<0.001
Satisfactory (Y3, Z2, Z3)	78	69	-
Acceptable (X2, X3, Y2)	3	3	-
Poor (X1, Y1, Z1)	0	13	-
Cement leakage			0.09
Posterior	3	0	-
Cranial	2	2	-
Anterior	4	3	-
Caudal	1	5	-
Lateral	6	15	-
Need for revision	1	0	-
Total, n (%)	16 (21)	25 (29)	-

<sup>a</sup>Fisher exact test.

**Table 3.** Radiation exposure data comparison in the 2 groups.

Variable	O-arm Group (n = 62)	Surgivisio Group (n = 61)	P Value <sup>a</sup>
2D imaging duration, s	25.99 ± 15.35 (7.17–84.87)	32.66 ± 20.06 (9–156)	0.04
No. of 3D acquisitions/patient	1.63 ± 0.96 (1–5)	1.01 ± 0.30 (1–2)	<0.001
Dose-length product, mGy-cm	622 ± 454 (88–2155)	-	-
Overall DAP, mGy-cm <sup>2</sup>	-	5326 ± 4180 (1258–25,090)	-
DAP related to 2D, mGy-cm <sup>2</sup>	10,222 ± 93,306 (1173–63,331)	2294 ± 2524 (344–13,298)	<0.001
Overall effective dose, mSv	11.47 ± 7.32 (2.92–33.59)	1.14 ± 0.67 (0.42–4.08)	<0.001
Effective dose per level, mSv	9.83 ± 6.94 (1.82–33.59)	0.88 ± 0.47 (0.24–2.82)	<0.001
Effective dose related to 2D, mSv	2.24 ± 1.80 (0.10–7.32)	0.47 ± 0.41 (0.12–2.57)	<0.001
Effective dose related to 3D, mSv	9.22 ± 6.78 (1.31–32.33)	0.67 ± 0.37 (0.22–2.18)	<0.001
Effective dose per 3D acquisition, mSv	5.84 ± 3.12 (1.31–12.56)	0.60 ± 0.27 (0.22–1.33)	<0.001
Effective dose related to 2D calculated with <i>w</i> <sup>b</sup> , mSv	2.39 ± 2.19 (0.22–14.25)	0.57 ± 0.66 (0.07–3.46)	<0.001
Absolute risk of radiation-induced cancer equivalent to a whole-body exposure, %	$4.9 \times 10^{-4} \pm 3.5 \times 10^{-4}$ ( $9.1 \times 10^{-5} - 1.7 \times 10^{-3}$ )	$5.7 \times 10^{-5} \pm 3.4 \times 10^{-5}$ ( $2.2 \times 10^{-5} - 2.0 \times 10^{-4}$ )	<0.001

Abbreviations: 2D, 2-dimensional; 3D, 3-dimensional; DAP, dose-area product; E, effective dose.

Note: Results are expressed as mean ± SD (range) in their respective units.

<sup>a</sup>Student *t* test.<sup>b</sup>*w* is the conversion factor used to calculate the effective dose from the DAP: 0.19 for thoracic and 0.26 mSv/Gy-cm<sup>2</sup> for lumbar spine.<sup>17</sup>

equivalent to a whole-body irradiation was also calculated, considering a value of 5% per Sv.<sup>18</sup> Operative and imaging duration per level were also calculated. The vertebral filling was radiologically appreciated using the Garnier classification<sup>19</sup> and quoted as satisfactory (Y3, Z2, Z3), acceptable (X2, X3, Y2), or poor (X1, Y1, Z1). Cement leakage was classified as anterior, cranial, posterior, lateral, or caudal.

### Outcome Measures

The main outcome was the overall effective dose; the secondary outcomes were the effective dose per 3D acquisition and received by the surgeon during 2D fluoroscopy, AR, the operative and imaging durations, the image quality in 2D and 3D, and the vertebral cement filling.

### Statistical Methods

Statistical analyses were performed using R statistical software,<sup>20</sup> v.3.1.3. Student *t* test was used for comparison of numerical variables, and Fisher exact test was used for binomial comparison. Correlations were determined using the Pearson test and analysis of variance. A threshold ≤0.05 was defined as a statistically significant difference.

## RESULTS

### Demographic Data

A total of 123 patients were included: 62 in the O-arm group and 61 in the Surgivisio group. Sex ratio (men/women) was 24/38 for the O-arm group and 24/37 for the Surgivisio group. A total of 166 vertebrae were operated: 81 in the O-arm group and 85 in the Surgivisio group. Magerl repartition was as follows: 65 (86%)

A1, 6 (8%) A2, and 10 (13%) A3 in the O-arm group; 77 (90%) A1, 5 (6%) A2, and 3 (4%) A3 in the Surgivisio group.

### Operative Data

There was a significantly higher operative time in the O-arm group compared with that in the Surgivisio group, with a mean duration of 34.52 vs 30.12 minutes, respectively (*P* = 0.04). The same trend was observed for the mean operative time per level: 28.75 vs 24.16 minutes, respectively (*P* = 0.01). Unipedicular approach during vertebroplasty was achieved for 34 (42%) procedures in the O-arm group and 69 (81%) procedures in the Surgivisio group, with a significant difference (*P* < 0.001). More procedures were performed by junior surgeons in the O-arm group (*P* = 0.02). These data are detailed in Table 1.

### Radiological Results

For the 2D fluoroscopic duration, an average of 25.99 seconds for the O-arm group and 32.66 seconds for the Surgivisio group were observed, with a significant

**Table 4.** Correlation of the effective dose and surgeon level with other parameters for the 2 groups.

Variable Comparison	O-arm Group (n = 62) P Value	Surgivisio Group (n = 61) P Value
Effective dose and age <sup>a</sup>	0.02	0.79
Effective dose and body mass index <sup>a</sup>	0.07	0.16
Effective dose and operative time <sup>a</sup>	0.3	<0.001
Effective dose and imaging duration <sup>a</sup>	<0.001	0.45
Effective dose and surgeon level <sup>b</sup>	0.28	0.17
Surgeon level and operative time <sup>b</sup>	0.73	0.12

<sup>a</sup>Pearson correlation test.<sup>b</sup>Analysis of variance method.

difference ( $P = 0.04$ ). Vertebral filling was significantly better in the O-arm group, with 100% of satisfactory and acceptable results vs 85% in the Surgivision group ( $P < 0.001$ ). Cement leakage was less frequent but not significant in the O-arm group, with 16 (20%) vs 25 (29%) reported in the Surgivision group ( $P = 0.09$ ), with a posterior leakage requiring immediate decompression in the O-arm group. All operative data are detailed in Table 2.

### Radiation Exposure

The overall effective dose was significantly higher in the O-arm group compared with the Surgivision group, with a mean of 11.47 vs 1.14 mSv, respectively ( $P < 0.001$ ). The same trend was found for the effective dose per level: 9.83 vs 0.88 mSv, respectively ( $P < 0.001$ ). The 3D-related effective dose was significantly higher in the O-arm group, with a mean of 9.22 vs 0.67 mSv in the Surgivision group ( $P < 0.001$ ). The same effect was observed for the effective dose per 3D acquisition: 5.84 vs 0.60 mSv, respectively ( $P < 0.001$ ), and for the 2D-related effective dose: 2.25 vs 0.47 mSv, respectively ( $P < 0.001$ ). The comparison between the effective dose related to 2D calculated with PCXMC and with the European Commission  $w$  conversion factors found similar results of 2.25 vs 2.40 mSv, respectively, for the O-arm group ( $P = 0.68$ ), and the same trend for the Surgivision group, with a mean of 0.47 vs 0.57 mSv, respectively ( $P = 0.30$ ). In the O-arm group, more 3D acquisitions were performed than in the Surgivision group: a mean of 1.63 acquisitions per patient vs 1.01, respectively, with a significant difference ( $P < 0.001$ ). Overall AR followed the same trend, with a mean of  $4.9 \times 10^{-4}\%$  with the O-arm group and  $5.7 \times 10^{-5}\%$  with the Surgivision group ( $P < 0.001$ ). Irradiation data are detailed in Table 3.

### Correlation Study

Correlation studies revealed that the effective dose was not correlated to the surgeon level ( $P = 0.24$  and  $0.17$ , respectively) but only to the age and the imaging duration in the O-arm group ( $P = 0.02$  and  $P < 0.001$ , respectively) and to the operative time in the Surgivision group ( $P < 0.001$ ). The analysis of variance method showed no correlation between surgeon level and operative time in both groups ( $P = 0.61$  and  $P = 0.12$ , respectively). Correlation studies are detailed in Table 4.

### Image Quality

Image quality always was sufficient in 3D for both groups and significantly better in 2D for the O-arm group than for the Surgivision group ( $P = 0.01$ ). These results are summarized in Table 5.

**Table 5.** Subjective image quality.

Image Quality	O-arm Group	Surgivision Group	P Value <sup>a</sup>
3-Dimensional			1
Acceptable	62	61	-
Insufficient	0	0	-
2-Dimensional			0.01
Acceptable	62	54	-
Insufficient	0	7	-

<sup>a</sup>Fisher exact test.

## DISCUSSION

The most important finding was the confirmation of most hypotheses with significantly more irradiation with the O-arm in comparison with the Surgivision device, with a mean 10 times higher radiation exposure. To our knowledge, this is the first time that a comparative study between the O-arm and Surgivision devices was conducted in clinical practice. However, Rousseau et al performed a dosimetric comparison in experimental conditions.<sup>21</sup> The authors found an effective dose related to 3D of 2.41 and 0.35 mSv with the O-arm and Surgivision device, respectively, and an effective dose related to 2D of 1.54 and 0.30 mSv, respectively. They also reported that organ doses were 5 to 7 times higher with the O-arm in comparison with the Surgivision device, which followed a trend that aligned with our results.

The first prospective series about kyphoplasty under O-arm guidance was performed by Schils on 16 cases.<sup>22</sup> He reported an operative time of 41 minutes, a fluoroscopy time of 3.23 minutes, and a fluoroscopy time per level of 2.43 minutes. The same author published about 54 cases<sup>23</sup> with reduced durations: operative time of 38 minutes, fluoroscopy time of 3.1 minutes, and fluoroscopy time per level of 2.5 minutes. Tonetti et al published the first series<sup>9</sup> of 65 consecutive vertebroplasties using the Surgivision device and found a mean operative time of 30 minutes. Other 3D devices were used for percutaneous cementoplasty. Tam et al utilized the Axiom Artis dTA VB31 (Siemens, Germany) and found a mean operative time of 64 minutes.<sup>24</sup> Sing and Jeong used the Siremobil isoC3D (Siemens, Germany) and reported a mean operative time of 52 minutes.<sup>25</sup> Ruatti et al performed 72 percutaneous procedures under the guidance of the Arcadis Orbic System (Siemens, Germany) and found a mean operative time by level of 46 minutes.<sup>26</sup>

Absence of correlation between operative time and surgeon level for the 2 groups indicated that the step-by-step process included in the O-arm navigation and in the Surgivision systems helped to standardize the surgical technique.



Izadpanah et al reported results about 30 computer-navigated kyphoplasties on the thoracic spine (TS) and the lumbar spine (LS).<sup>27</sup> They found an average operation time of 67 minutes in the TS and 62 minutes in the LS, a radiation time of 99 seconds in the TS and 74 seconds in the LS, with a DAP of 12,450 and 13,180 mGy·cm<sup>2</sup>, respectively. Tonetti et al<sup>9</sup> found a mean E of 1.32 mSv per level, with the use of the Surgivisio device. However, they utilized European Commission conversion factors *w* for dose calculation. These results are less accurate than with the use of the PCXMC software,<sup>17</sup> with an uncertainty in practice about 10% to 20%. They found similar results than the current study when compared with those obtained with the same conversion factors. Another case reported an effective dose of 1.17 mSv for the use of a 180-image 3D acquisition with the Surgivisio device, in the case of a T1 vertebra osteoid osteoma resection.<sup>10</sup> Another study from Boudissa et al about percutaneous pedicle screw insertion using the Surgivisio device<sup>11</sup> found a mean effective dose of 1.97 mSv. The study from Farah et al<sup>28</sup> about pedicle screw insertion using the O-arm and the AIRO (Brainlab AG, Germany) devices found a mean effective dose of 1.04 and 3.9 mSv, respectively, per navigated vertebra, with 2D imaging used only for landmarking.

Differences between O-arm and Surgivisio may be explained by technological aspects. The O-arm is a 2D and 3D cone beam computerized tomography. The Surgivisio is a 2D and 3D C-arm. Both devices use plan detectors as imaging technology. However, the O-arm performs a 3D acquisition with delivery of 192 images, whereas the Surgivisio could perform 180 or 90 images for a whole 3D acquisition, explaining higher effective dose related to 3D in the O-arm group. Voltage is higher in standard O-arm settings in comparison with the Surgivisio device, leading to higher level of irradiation.<sup>21</sup> Higher effective dose and better image quality in 2D mode for the O-arm can be explained by its settings, with a standard 30 pulses per second. Surgivisio produces 8 pulses per second in 2D mode. The O-arm is already known to produce high exposure in 2D.<sup>29,30</sup> Operative time reduction in the Surgivisio group may be related to the easy way to put the reference frame on the patient on both LS and TS. Thoracic O-arm cementoplasty may require a spinous clamp with skin incision and muscular dissection around the spinous process before performing the 3D acquisition, increasing the operative duration. Repeated 3D acquisitions increased operative time and also effective dose related to 3D. Putting in perspective the absence of poor radiologic cement

filling and less cement leakage in the O-arm group, we could suppose that the better image quality may have improved control of cement injection during O-arm procedures. Higher number of kyphoplasties in the O-arm group may have also helped reducing the rate of cement leakage.<sup>31</sup> Additionally, higher age in the O-arm group could lead to poor bone quality and difficulty to clearly see vertebrae during cementoplasty due to osteopenia. Better radiological results were reached by higher necessary irradiation to get adequate image quality. Higher rate of unipedicular vertebroplasties in the Surgivisio group could also explain its inferior radiological results.

According to the as low as reasonably achievable principle,<sup>32</sup> there are several ways to decrease dose regarding the results with the O-arm. Using the low-dose mode in 3D, limiting the number of 3D and 2D acquisitions and finally using the collimation of the imaging field may help to decrease the overall dose. For the Surgivisio group, using the 90-image 3D acquisition mode and limiting the number of 3D and 2D acquisitions may also decrease the overall dose.

There were some limitations in this study: its ambispective design was the first; the Surgivisio cohort may have benefited from a Hawthorne effect<sup>33</sup> in contrast to the retrospective part of the ambispective O-arm cohort. Second, the effective dose calculation is an estimation using standard and specific measurements for the Monte Carlo simulation. There was a calculation bias in the dose estimation because we could not intraoperatively measure the exact focus to skin distance in clinical practice, considering this distance modifying every time during the surgery and even more during the 3D acquisition with the Surgivisio device. For reproducibility purposes, we considered the standard focus to skin distance of 80 cm for all patients in the 2 groups, according to standard settings of the software. So, the accuracy of the dose estimation could be supported by the consideration of the other parameters.

## CONCLUSION

The O-arm delivered a 10 times higher effective dose during navigated cementoplasty procedures in comparison with the Surgivisio device. Operative time was also higher with the O-arm, while image quality and radiological results were better. Further studies about other minimally invasive spine techniques comparing these devices should be performed to help spine surgeons to determine the best choice for their clinical practice.



## REFERENCES

1. Taylor RS, Taylor RJ, Fritzell P. Balloon kyphoplasty and vertebroplasty for vertebral compression fractures: a comparative systematic review of efficacy and safety. *Spine (Phila Pa 1976)*. 2006;31(23):2747–2755. doi:10.1097/01.brs.0000244639.71656.7d
2. Zhu Y, Cheng J, Yin J, Zhang Z, Liu C, Hao D. Therapeutic effect of kyphoplasty and balloon vertebroplasty on osteoporotic vertebral compression fracture: a systematic review and meta-analysis of randomized controlled trials. *Medicine (Baltimore)*. 2019;98(45):e17810. doi:10.1097/MD.00000000000017810
3. Muto M, Guarnieri G, Giurazza F, Manfrè L. What's new in vertebral cementoplasty? *Br J Radiol*. 2016;89(1059):20150337. doi:10.1259/bjr.20150337
4. Laine T, Lund T, Ylikoski M, Lohikoski J, Schlenszka D. Accuracy of pedicle screw insertion with and without computer assistance: a randomised controlled clinical study in 100 consecutive patients. *Eur Spine J*. 2000;9(3):235–240. doi:10.1007/s005860000146
5. National Research Council. *Health Risks from Exposure to Low Levels of Ionizing Radiation: BEIR VII Phase 2*. National Academies Press; 2006.
6. Tonetti J, Boudissa M, Kerschbaumer G, Seurat O. Role of 3D intraoperative imaging in orthopedic and trauma surgery. *Orthop Traumatol Surg Res*. 2020;106(1S):S19–S25. doi:10.1016/j.otsr.2019.05.021
7. Zygourakis CC, DiGiorgio AM, Crutcher CL, et al. The safety and efficacy of CT-guided, fluoroscopy-free vertebroplasty in adult spinal deformity surgery. *World Neurosurg*. 2018;116:e944–e950. doi:10.1016/j.wneu.2018.05.139
8. Wardlaw D, Van Meirhaeghe J, Ranstam J, Bastian L, Boonen S. Balloon kyphoplasty in patients with osteoporotic vertebral compression fractures. *Expert Rev Med Devices*. 2012;9(4):423–436. doi:10.1586/erd.12.27
9. Tonetti J, Boudissa M, Kerschbaumer G, Prod'Homme M. All-in-one intraoperative 3D imaging and navigation on percutaneous vertebroplasty. preliminary results on the first 51 patients. *EPIC Series in Health Sciences*. 2019;3:370–375. doi:10.29007/w6d6
10. Prod'homme M, Cavalié G, Kerschbaumer G, Valmary-Degano S, Boudissa M, Tonetti J. T1 vertebra pedicular osteoid osteoma: minimally invasive surgical resection aided by new integrated navigation to 3D imaging device. *Case Rep Orthop*. 2019;2019:7626454. doi:10.1155/2019/7626454
11. Boudissa M, Prod'homme M, Kerschbaumer G, Ruatti S, Tonetti J. 3D-imaging in percutaneous spine surgery using the Surgivisio system. *Orthop Traumatol Surg Res*. 2020;106(6):1183–1186. doi:10.1016/j.otsr.2020.01.018
12. Prod'homme M, Pour Jafar S, Zogakis P, Stutz P. A novel minimally invasive reduction technique by balloon and distractor for intra-articular calcaneal fractures: a report of 2 cases. *Case Rep Orthop*. 2018;2018:7909184. doi:10.1155/2018/7909184
13. Kerschbaumer G, Gaulin B, Ruatti S, Tonetti J, Boudissa M. Clinical and radiological outcomes in thoracolumbar fractures using the spinejack device. A prospective study of seventy-four patients with a two point three year mean of follow-up. *Int Orthop*. 2019;43(12):2773–2779. doi:10.1007/s00264-019-04391-1
14. Magerl F, Aebi M, Gertzbein SD, Harms J, Nazarian S. A comprehensive classification of thoracic and lumbar injuries. *Eur Spine J*. 1994;3(4):184–201. doi:10.1007/BF02221591
15. Tapiovaara MJ, Lakkisto M, Servomaa A. *PCXMC: A PC-Based Monte Carlo Program for Calculating Patient Doses in Medical X-Ray Examinations*. Helsinki, Finland: STUK; 1997.
16. Bongartz SJG G, Jurik AG, Leonardi M, van Persijn van Meerten E, Rodríguez R, Schneider K. *European Guidelines for Multislice Computed Tomography*. 2004. <http://www.drs.dk/guidelines/ct/quality/index.htm>. Accessed February 18, 2021.
17. European Commission. Radiation induced long-term health effects after medical exposure. *EU Scientific Seminar*. 2013. [https://ec.europa.eu/energy/sites/ener/files/documents/seminar\\_proceedings\\_radiation\\_protection\\_series\\_ndeg\\_rp182.pdf](https://ec.europa.eu/energy/sites/ener/files/documents/seminar_proceedings_radiation_protection_series_ndeg_rp182.pdf). Accessed February 18, 2021.
18. Wambersie A. The international commission on radiation units and measurements. *J ICRU*. 2005;5(2):ii–iii. doi:10.1093/jicru/ndi017
19. Garnier L, Tonetti J, Bodin A, et al. Kyphoplasty versus vertebroplasty in osteoporotic thoracolumbar spine fractures. short-term retrospective review of a multicentre cohort of 127 consecutive patients. *Orthop Traumatol Surg Res*. 2012;98(6 Suppl):S112–S119. doi:10.1016/j.otsr.2012.03.018
20. R Core Team. *R: A Language and Environment for Statistical Computing*. Vienna, Austria: R Foundation for Statistical Computing; 2019. <https://www.R-project.org/>.
21. Rousseau J, Dreuil S, Bassinet C, Cao S, Elleaume H. Surgivisio® and O-arm®O2 cone beam CT mobile systems for guidance of lumbar spine surgery: comparison of patient radiation dose. *Phys Med*. 2021;85:192–199. doi:10.1016/j.ejmp.2021.04.018
22. Schils F. O-arm guided balloon kyphoplasty: preliminary experience of 16 consecutive patients. *Acta Neurochir Suppl*. 2011;109:175–178. doi:10.1007/978-3-211-99651-5\_27
23. Schils F. O-arm-guided balloon kyphoplasty: prospective single-center case series of 54 consecutive patients. *Neurosurgery*. 2011;68(2 Suppl Operative):s250–s266. doi:10.1227/NEU.0b013e31821421b9
24. Tam AL, Mohamed A, Pfister M, et al. C-arm cone beam computed tomography needle path overlay for fluoroscopic guided vertebroplasty. *Spine (Phila Pa 1976)*. 2010;35(10):1095–1099. doi:10.1097/BRS.0b013e3181bc39c6
25. Shin JH, Jeong JH. Preliminary report of three-dimensional reconstructive intraoperative C-arm in percutaneous vertebroplasty. *J Korean Neurosurg Soc*. 2012;51(2):120–123. doi:10.3340/jkns.2012.51.2.120
26. Ruatti S, Dubois C, Chipon E, et al. Interest of intraoperative 3D imaging in spine surgery: a prospective randomized study. *Eur Spine J*. 2016;25(6):1738–1744. doi:10.1007/s00586-015-4141-5
27. Izadpanah K, Konrad G, Südkamp NP, Oberst M. Computer navigation in balloon kyphoplasty reduces the intraoperative radiation exposure. *Spine (Phila Pa 1976)*. 2009;34(12):1325–1329. doi:10.1097/BRS.0b013e3181a18529
28. Farah K, Coudert P, Graillon T, et al. Prospective comparative study in spine surgery between O-arm and AIRO systems: efficacy and radiation exposure. *World Neurosurg*. 2018;118:e175–e184. doi:10.1016/j.wneu.2018.06.148
29. Pitteloud N, Gamulin A, Barea C, Damet J, Racloz G, Sans-Merce M. Radiation exposure using the O-arm® surgical imaging system. *Eur Spine J*. 2017;26(3):651–657. doi:10.1007/s00586-016-4773-0
30. Prod'homme M, Sans-Merce M, Pitteloud N, Damet J, Lascombes P. Intraoperative 2D C-arm and 3D O-arm in children: a

comparative phantom study. *J Child Orthop*. 2018;12(5):550–557. doi:10.1302/1863-2548.12.180016

31. Wang H, Sribastav SS, Ye F, et al. Comparison of percutaneous vertebroplasty and balloon kyphoplasty for the treatment of single level vertebral compression fractures: a meta-analysis of the literature. *Pain Physician*. 2015;18(3):209–222. doi:10.36076/ppj/2015.18.209

32. National Council on Radiation Protection and Measurements. *Report No. 107. Implementation of the Principle of as Low as Reasonably Achievable (ALARA) for Medical and Dental Personnel*. NCRP Publications; 1990.

33. Demetriou C, Hu L, Smith TO, Hing CB. Hawthorne effect on surgical studies. *ANZ J Surg*. 2019;89(12):1567–1576. doi:10.1111/ans.15475

**Funding:** The authors received no financial support for the research, authorship, and/or publication of this article.

**Declaration of Conflicting Interests:** The authors report no conflicts of interest in this work.

**Disclosures:** Marc Prod'homme, Guillaume Cavalié and Didier Grasset have nothing to disclose. Jérôme Tonetti discloses that he is on the speaker's bureau of the eCential Robotics company and received consulting honorarium from; he is on the speaker's bureau for the Spine Art company and received money for consulting from, and he also received a fellowship support from the Zimmer Biomet company. Duccio Boscherini discloses that he was on the speaker's bureau for the Medtronic company, and he still remains a non-remunerated consultant; he was also on the speaker's bureau for the Johnson and Johnson

company and received money for consulting from. Gael Kerschbaumer discloses that he is a consultant for the eCential Robotics company and received grants for research from. Mehdi Boudissa discloses that he is on the speaker's bureau as a consultant for the eCential Robotics company received grants for research from; he also received grants for a fellowship training from the Zimmer Biomet company.

**Patient consent for publication:** Patient's anonymity was protected and all patients signed an informed written consent before enrollment in the study.

**Ethical Standards:** The procedures followed were in accordance with the ethical standards of the responsible committees on human experimentation (institutional and national) and with the Helsinki Declaration of 1975, as revised in 2000. The ethical commission on human research of the Vaud canton approved the research protocol (Nr. 2021-00298).

**Corresponding Author:** Marc Prod'homme, Clinic La Source, Neuro Orthopedic Center, Ave Jomini 8, CH-1004 Lausanne, Switzerland; marcprod86@gmail.com

This manuscript is generously published free of charge by ISASS, the International Society for the Advancement of Spine Surgery. Copyright © 2022 ISASS. To see more or order reprints or permissions, see <http://ijssurgery.com>.